


Quantitative Depth Profile (QDP) Analysis of Cr Marker in Alumina Sample

GDS Applications Lab • LECO Corporation, Saint Joseph, Michigan USA

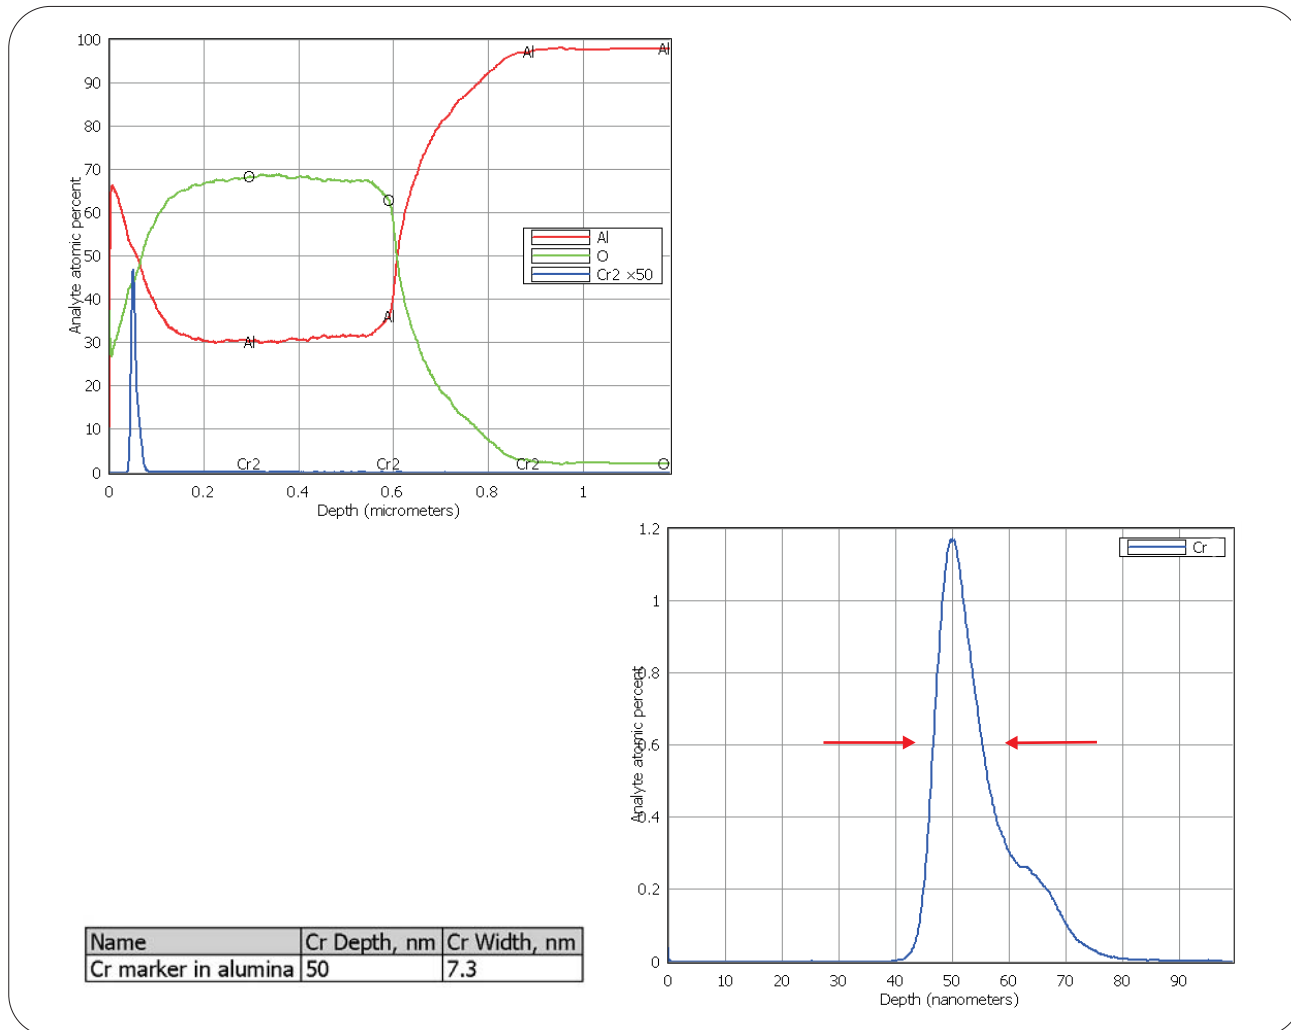

Parameters

Grimm-Style RF 4 mm Lamp
 20 W, 1000 V
 40 s, 1000/s

For questions on this analysis e-mail us at:
info@leco.com

For a complete listing of snapshots and performance notes visit us on the web at www.leco.com in the Spectroscopy section of the Applications Library.

